


MASS SPECTROMETRY REPORT

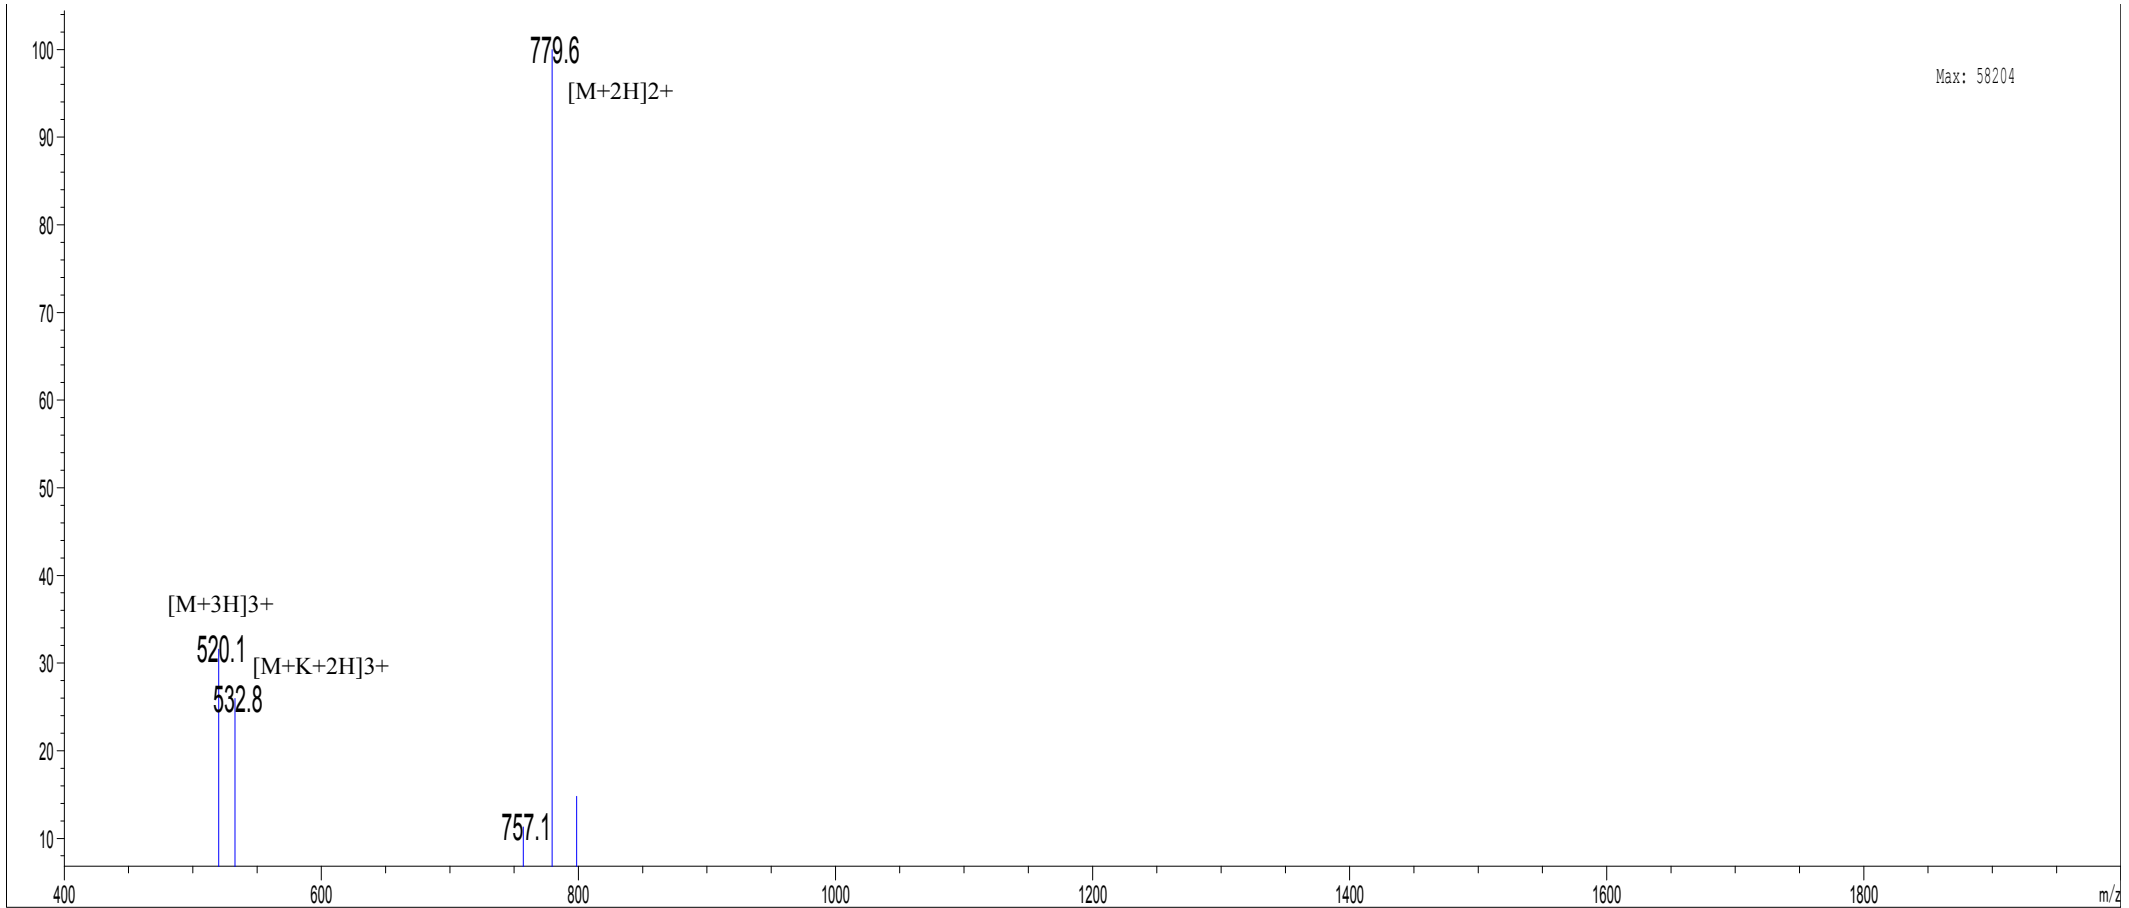

Sample Description

Analyzed date: 2025-07-11
Analyst: YU
Sample: 同位素标记牛 II 型 GR-18
M.W.: 1557.68
Lot. No.: P250627-SJ1271769

Instrument

Agilent-6125B
Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp.: 250 °C
Block Temp.: 200 °C

Probe Bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. Conc.: 50%H₂O/50%ACN